

[To be published in the Gazette of India, Part II, Section 3, Sub-section (ii)]

Government of India

Ministry of Consumer Affairs, Food and Public Distribution

Department of Consumer Affairs

New Delhi, Dated the 25.6.2016

Notification

S.O.— Whereas the Central Government, after considering the report submitted to it by the prescribed authority, is satisfied that the model described in the said report is in conformity with the provisions of the Legal Metrology Act, 2009 (1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;

Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, the Central Government hereby issues and publishes the certificate of approval of the model of non-automatic weighing instrument with digital indication of medium accuracy (accuracy class-III) of series "ECON" and with brand name "EAGLE" (here after in this notification referred to as the said model), manufactured by M/s E. G. Kantawalla Pvt. Ltd., Survey No 28/1, Damodar Nagar, Old Nagar, Mundhwa Road, Kharadi, Pune-411014 and which is assigned the approval mark IND/09/16/490 (the picture of model is given below as figure 1);

The said model is a strain gauge type load cell based non-automatic weighing instrument with a maximum capacity of 35kg and minimum capacity of 20g. The verification scale interval (e) is 1g upto 10kg, above 10kg & upto 20kg is 2g and above 20kg & upto 35kg is 5g. It has tare device with a 100 percent tare. The light emitting diode (LED) display indicates the weighing result. The instrument operates on 230Volts, 50Hertz alternating current power supply. It is used as table top type weighing instrument.

Figure 1.



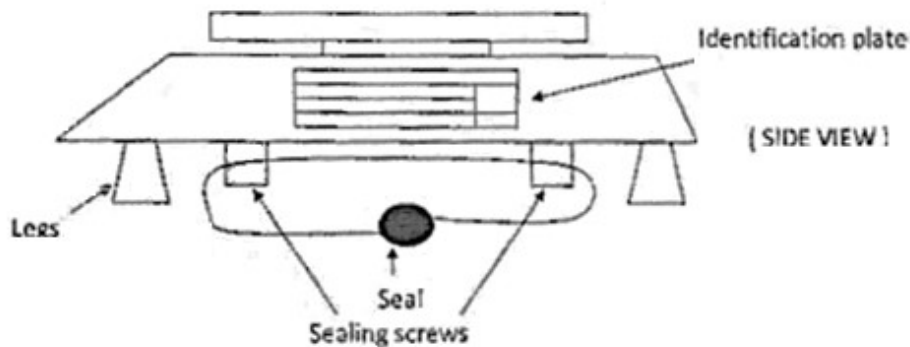


Figure.2

The sealing provision for the weighing instrument is provided by two body fitting screws as shown above in figure 2. A dip switch is provided in the printed circuit board to disable access to external calibration control.

Further, in exercise of the powers conferred by sub-rule (9) of rule 8 of the Legal Metrology (Approval of Models) Rules, 2011, the Central Government hereby declares that this certificate of approval of the said model shall also cover the weighing instruments of similar make, accuracy and performance of same series with maximum capacity up to 50kg with number of verification scale interval (n) in the range of 100 to 10000 for 'e' value of 100mg to 2g and with number of verification scale interval (n) in the range of 500 to 10000 for 'e' value of 5g or more and with 'e' value of 1×10^k , 2×10^k or 5×10^k , where k is a positive or negative whole number or equal to zero manufactured by the same manufacturer in accordance with the same principle, design and with the same materials with which, the said approved model has been manufactured.

[F.No.WM-21(275)2016]

Babu Nishant

(B. N. Dixit)

Director (Legal Metrology) to Government of India